

# Protocols for Laboratory Verification of Performance of the FilmArray® Gastrointestinal (GI) Panel

TECHNICAL  
::: NOTE

## Purpose

---

The Clinical Laboratory Improvement Amendments (CLIA), passed in 1988, establishes quality standards for all laboratory testing to ensure the accuracy and reliability of patient test results, regardless of where the test is performed. The CLIA regulations include a requirement for verifying the performance specifications of unmodified, moderate complexity tests cleared or approved by the FDA.

This document provides examples of verification procedures to assist your laboratory in developing a protocol for the verification of the FilmArray GI Panel performance on FilmArray® 1.5, 2.0 and Torch Systems as required by CLIA. Several possible verification schemes, compatible with the FilmArray GI Panel, have been designed. Each scheme provides positive and negative tests for each organism detected by the FilmArray GI Panel using non-clinical specimens and may be easily modified or expanded to meet specific criteria. Day-to-day variation is evaluated by testing each sample on two separate days. To evaluate user-to-user variation, multiple laboratory technicians may test the same sample. In addition, testing patient samples for verification or to evaluate matrix effects on the performance of the FilmArray GI Panel should be done under the guidance of the Laboratory Director, but is not described here. As per the CLIA regulation, the Laboratory Director is ultimately responsible for ensuring that verification procedures meet the appropriate standards for CLIA and applicable laboratory accrediting agencies.

## FilmArray Intended Use

---

The FilmArray GI Panel is a multiplexed nucleic acid test intended for use with FilmArray Systems for the simultaneous qualitative detection and identification of multiple gastrointestinal viral, parasitic and bacterial nucleic acid targets in stool samples in Cary Blair transport media obtained from individuals suspected of gastrointestinal tract infections. The following organisms and subtypes are identified using the FilmArray GI Panel:

*Campylobacter* spp. (*C. jejuni*, *C. coli*, and *C. upsaliensis*), *Clostridium difficile* toxin A/B, *Plesiomonas shigelloides*, *Salmonella* spp., *Vibrio* spp. (*V. parahaemolyticus*, *V. vulnificus*, and *V. cholerae*), *Yersinia enterocolitica*, Enteroaggregative *E. coli* (EAEC), Enteropathogenic *E. coli* (EPEC), Enterotoxigenic *E. coli* (ETEC) *lt/st*, Shiga-like toxin-producing *E. coli* (STEC) *stx1/stx2*, *E. coli* O157, *Shigella*/Enteroinvasive *E. coli* (EIEC), *Cryptosporidium*, *Cyclospora cayetanensis*, *Entamoeba histolytica*, *Giardia lamblia*, adenovirus F 40/41, astrovirus, norovirus GI/GII, rotavirus A, and sapovirus (I, II, IV, and V).

The complete intended use statement and additional information about the use of the FilmArray System can be found in the *FilmArray GI Panel Instruction Booklet*.

## Performance Verification: Overview

Each procedure described below will generate multiple positive and negative results for each of the organisms targeted by the FilmArray® Gastrointestinal (GI) Panel. The procedures were developed using a NATrol™ GI Panel available from ZeptoMetrix Corporation, Buffalo, NY (part number NATGIP-BIO).

Two different examples of performance verification procedures are described: (1) a simple protocol for the verification the GI Panel in a synthetic background (Negative) provided with the ZeptoMetrix NATrol™ Control Organism and (2) a simple Cary Blair Media protocol that evaluates the performance of each assay on the GI Panel with a stool in Cary Blair sample matrix.

A FilmArray® System is defined as all FilmArray® Instruments or modules that are connected to and controlled by a single computer system. If the laboratory director chooses not to verify the instruments individually, it is advised that test replicates are evenly distributed among the instruments or modules.

The procedures have been designed to take advantage of the multiplex nature of the FilmArray GI Panel. Verification testing efficiency is maximized by evaluating multiple target organisms in a single test run.

Clinical/patient specimens may be used in place of or in addition to the verification schemes described here in order to assess clinical sensitivity and sample matrix effects in its performance verification of the FilmArray GI Panel.

## TECHNICAL ::: NOTE

**Table 1.** Overview of Verification Protocols

Verification Protocol	Organisms per Pool <sup>a</sup>	Number of Sample Pools	Replicates per Sample Pool	Pouches Required	Expected Positive Results	Expected Negative Results	Approximate Days of Testing <sup>b</sup>
Example 1: Simple protocol	5 or 6	4	4	16	4 per organism	12 per organism	4
Example 2: Stool in Cary Blair protocol	5 or 6	4	4	16	4 per organism	12 per organism	4

<sup>a</sup> Depending on the material used for verification, pooling of organisms may not be appropriate and the values in the table may need to be modified.

<sup>b</sup> The approximate number of days for testing assumes a system configured with one instrument.

## Performance Verification: Materials

The following materials may be used to perform verification procedures:


**Table 2.** Materials needed for recommended protocols

Material	Part Number
FilmArray GI Panel Kit (30 tests)	Biofire Diagnostics, LLC RFIT-ASY-0116
Control Organism	ZeptoMetrix NATGIP-BIO <sup>a</sup>
Cary Blair Transport Media	Thermo Scientific Part # 23-005-47 (or equivalent)
5mL sample tubes	VWR Part # 89497-740 (or equivalent)
Transfer pipettes	VWR Part # 13-711-43 (or equivalent)

<sup>a</sup>Any appropriate source of organism may be used for verification of any or all of the assays in the FilmArray GI Panel. However, when alternate organism sources are used (i.e. not the ZeptoMetrix material), the sample volumes or pooling schemes suggested in the examples below may need to be adjusted.

### Simple Protocol

The simple protocol utilizes samples prepared by pooling together either 5 or 6 different organisms (ZeptoMetrix NATGIP-BIO control organism). The proposed pooling scheme (Table 3) should be followed to obtain the expected positive and negative results for each assay in a time and resource-efficient manner.

 **Note:** Dilution of ZeptoMetrix GI Verification Panel organisms beyond levels proposed in these guidelines may lead to inconsistent results and is not recommended.

The Simple Protocol can be followed to test a total of 16 pouches, providing 4 positive results and 12 negative results per organism. The number of samples tested per day should be determined by the individual laboratory. This testing scheme can be modified to run more samples per day based on the number of instruments in the FilmArray® System.

**Table 3.** Recommended Organism Pooling Scheme

Organism	Organism Volume	Negative Or Stool in Cary-Blair Media	Approximate Final Volume of Pool
<b>Pool 1</b>			
Enteraggregative <i>E. coli</i> (EAEC)	0.25 mL	0.85mL	2.1mL
Adenovirus Type 41	0.25 mL		
<i>Cryptosporidium parvum</i>	0.25 mL		
<i>Salmonella typhimurium</i>	0.25 mL		
Sapovirus	0.25 mL		
<b>Pool 2</b>			
Enteropathogenic <i>E. coli</i> (EPEC)	0.25 mL	0.85mL	2.35mL
Norovirus GI	0.25 mL		
Norovirus GII	0.25 mL		
<i>Cyclospora cayetanensis</i>	0.25 mL		
<i>Shigella sonnei</i>	0.25 mL		
Astrovirus	0.25 mL		
<b>Pool 3</b>			
Enterotoxigenic <i>E. coli</i> (ETEC) <i>lt/st</i>	0.25 mL	0.85mL	2.35mL
<i>Entamoeba histolytica</i>	0.25 mL		
<i>Clostridium difficile</i>	0.25 mL		
<i>Vibrio cholerae</i>	0.25 mL		
<i>Campylobacter jejuni</i>	0.25 mL		
<i>Campylobacter coli</i>	0.25 mL		
<b>Pool 4</b>			
<i>E. coli</i> O157	0.25 mL	0.85mL	2.1mL
Rotavirus	0.25 mL		
<i>Giardia lamblia</i>	0.25 mL		
<i>Plesiomonas shigelloides</i>	0.25 mL		
<i>Yersinia enterocolitica</i>	0.25 mL		


## TECHNICAL ::: NOTE

## Simple Protocol Example


The estimated total time to completion for this verification example is 4 days for systems configured with one instrument.

### Day 1

1. Prepare one sample pool (i.e. pool 1) from ZeptoMetrix NATGIP-BIO control material. An example organism pooling scheme is presented in Table 3.

 **Note:** It is important to prepare only the number of organism sample pools that will be tested within 3 days of preparation. The number of samples prepared may be increased or decreased based on the laboratory's work schedule and the number of instruments connected within a FilmArray® System.

- a. Use a transfer pipette to remove entire contents of a vial of ZeptoMetrix Negative (approximately 0.85mL) and transfer it to a tube large enough (at least 3mL) to hold the entire organism pool volume.
  - b. Use a transfer pipette to remove the entire contents of the ZeptoMetrix organism vial (approximately 0.25mL) and transfer to the larger tube containing the Negative diluent.
  - c. Repeat step b. for each of the remaining organisms to combine the appropriate organisms for each pool into a single vial or tube.
  - d. Ensure the pooled sample is effectively mixed by vortexing prior to removing a sample for testing.
  - e. Refrigerate samples (2–8°C) for up to 3 days for the evaluation of day-to-day variation.
2. Prepare and test 2 samples from a single sample pool (i.e. pool 1). The duplicate samples should be tested in a single day by different users.
  - 3.

 **Note:** For each sample, follow instructions in the *FilmArray® Gastrointestinal (GI) Panel Instruction Booklet* or *GI Panel Quick Guide* for pouch preparation, pouch hydration, sample loading, and sample testing.

4. Repeat steps 1 and 2 for the remaining sample pool (i.e. pool 2) to be tested that day.

### Day 2

To evaluate day-to-day variation, test the remaining samples (i.e. samples C and D) from the same sample pools prepared on Day 1 by repeating Step 2 above.

### Day 3


Prepare 2 new sample pools (i.e. pools 3 and 4) as described in Step 1. Test samples according to Step 2 (i.e. samples A and B) for each pool.

### Day 4

To evaluate day-to-day variation, test the samples prepared on Day 3 by repeating Step 2 (i.e. samples 3 and 4).

## TECHNICAL ::: NOTE


**Figure 1.** Simple protocol workflow

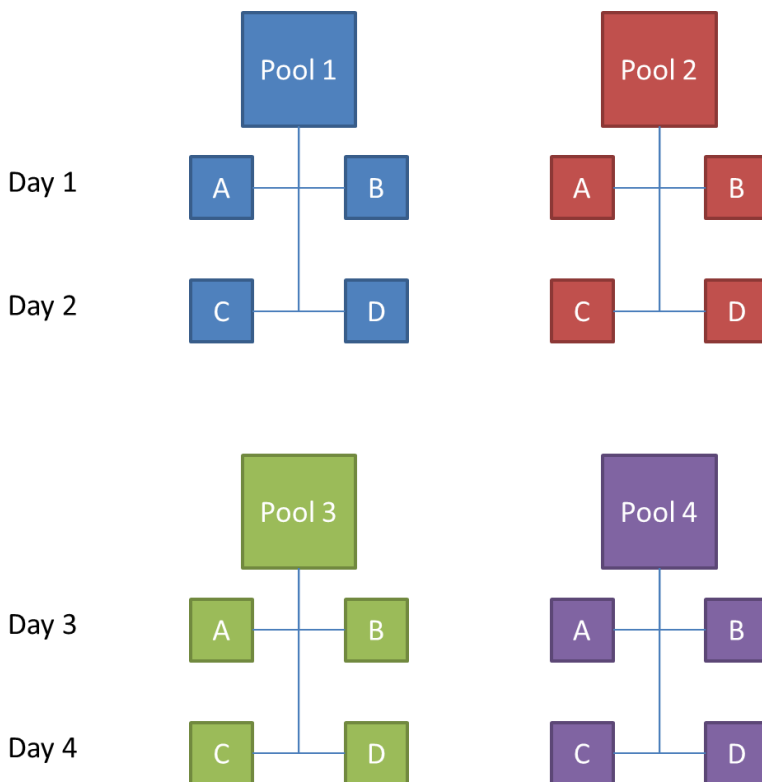

## TECHNICAL ::: NOTE

### Stool in Cary Blair Protocol

An example organism pooling scheme is presented above in Table 3. For this testing scheme, a stool sample in Cary Blair media will be used as the organism pool background rather than synthetic stool (Negative). The laboratory will require a stool sample in Cary Blair that is negative for all GI pathogens detected by the FilmArray® Gastrointestinal (GI) Panel. Laboratories may screen stool samples in Cary Blair with the FilmArray GI panel and select samples that yield all negative results as an appropriate background matrix for the pooling scheme. Pooled samples added to negative stool matrix can be stored overnight (or up to 3 days) at refrigeration temperature (2–8°C) for subsequent testing to evaluate day-to-day variation. Test replicates should be performed by different users to evaluate user to user variation.

 **Note:** Dilution of ZeptoMetrix GI Verification Panel organisms beyond levels proposed in these guidelines may lead to inconsistent results and is not recommended.


The Stool in Cary Blair Protocol can be followed to test a total of 16 pouches, providing 4 positive results and 12 negative results per organism. The number of samples tested per day should be determined by the individual laboratory. This testing scheme can be modified to run more samples per day based on the number of instruments in the FilmArray® System.

## Stool in Cary Blair Protocol Example


The estimated total time to completion for this verification example is 4 days for systems configured with one instrument.

### Day 1

1. Prepare one sample pool (i.e. pool 1) by mixing ZeptoMetrix NATGIP-BIO control material with a freshly prepared stool sample in Cary Blair transport media. An example organism pooling scheme is presented in Table 3.

 **Note:** It is important to prepare only the number of organism sample pools that will be tested within 3 days of preparation. The number of samples prepared may be increased or decreased based on the laboratory's work schedule and the number of instruments connected within a FilmArray® System.

- a. Use a transfer pipette to transfer approximately 0.85mL of a prepared stool in Cary Blair sample to a tube large enough (at least 3mL) to hold the entire organism pool volume.
  - b. Use a transfer pipette to remove the entire contents of the ZeptoMetrix organism vial (approximately 0.25mL) and transfer to the larger tube containing the stool sample.
  - c. Repeat with each of the remaining organisms to combine the appropriate organisms for each pool into a single vial or tube.
  - d. Ensure the pooled sample is effectively mixed by vortexing prior to removing a sample for testing.
  - e. Refrigerate samples (2–8°C) for up to 3 days for the evaluation of day-to-day variation.
2. Prepare and test two samples from a single sample pool (i.e. pool 1). The duplicate samples should be prepared consecutively and tested in a single day. For each sample:

 **Note:** Follow instructions in the *FilmArray® Gastrointestinal (GI) Panel Instruction Booklet* or *GI Panel Quick Guide* for pouch preparation, pouch hydration, sample loading, and sample testing.

3. Repeat Step 1 and 2 for the remaining sample pool (i.e. pool 2 to be tested that day).

### Day 2

To evaluate day-to-day variation, test the remaining samples (i.e. samples C and D) from the same sample pools prepared on Day 1 by repeating Step 2 above.

### Day 3


Prepare 2 new sample pools (i.e. pools 3 and 4) as described in Step 1. Test samples according to Step 2 (i.e. samples A and B) for each pool.

### Day 4

To evaluate day-to-day variation, test the samples prepared on Day 3 by repeating Step 2 (i.e. samples C and D).

## TECHNICAL ::: NOTE

**Figure 2.** Stool in Cary Blair media protocol workflow

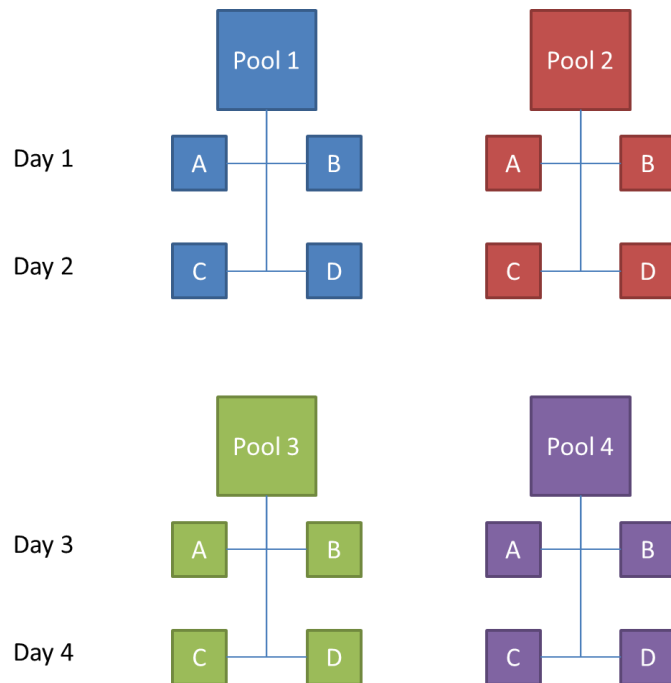

## TECHNICAL ::: NOTE

### Expanding the protocols

The protocols described above can be expanded by increasing the number of tests from each of the organism pools. Each organism pool contains enough material to complete up to 8 tests for each pool, doubling the number of tests described in the example protocols.

### Verification of Loaner and Repaired Instruments

If it becomes necessary to verify the performance of a loaner or repaired instrument, the following protocol may serve as a guideline but should be verified by the Laboratory Director

1. Select a few specimens and/or proficiency samples (any combination of positives and negatives) previously tested on the FilmArray® Gastrointestinal (GI) Panel. The Laboratory Director should determine the appropriate number of samples to test. Three to 6 samples may be sufficient. Proficiency samples should not be pooled or diluted.
2. Test the selected samples on the loaner or repaired instrument and document the results.

## Technical Support Contact Information

---

BioFire is dedicated to providing the best customer support available. If you have any questions or concerns about this process, please contact the FilmArray Technical Support team for assistance.

### **BioFire Technical Support**

Email: [support@biofiredx.com](mailto:support@biofiredx.com)

Phone: +1-801-736-6354, select Option 5



**TECHNICAL  
::: NOTE**



# FilmArray® Gastrointestinal (GI) Panel Verification Record

Computer System Serial #: \_\_\_\_\_

FilmArray GI Panel kit Part #: \_\_\_\_\_ Lot #: \_\_\_\_\_

Organism/sample Source and Lot #: \_\_\_\_\_

**TECHNICAL  
::: NOTE**

Organism	Instrument Serial #	Was the Organism Detected?	No. Positive	No. Negative	No. Days Tested	No. Users	Patient Samples Tested?
Enteroaggregative <i>E. coli</i> (EAEC)		<input type="checkbox"/> Yes <input type="checkbox"/> No					
Adenovirus F 40/41		<input type="checkbox"/> Yes <input type="checkbox"/> No					
<i>Cryptosporidium</i>		<input type="checkbox"/> Yes <input type="checkbox"/> No					
<i>Salmonella</i>		<input type="checkbox"/> Yes <input type="checkbox"/> No					
Sapovirus (I, II, IV, and V)		<input type="checkbox"/> Yes <input type="checkbox"/> No					
Enteropathogenic <i>E. coli</i> (EPEC)		<input type="checkbox"/> Yes <input type="checkbox"/> No					
Norovirus GI/GII		<input type="checkbox"/> Yes <input type="checkbox"/> No					
<i>Cyclospora cayetanensis</i>		<input type="checkbox"/> Yes <input type="checkbox"/> No					
<i>Shigella</i> / Enteroinvasive <i>E. coli</i> (EIEC)		<input type="checkbox"/> Yes <input type="checkbox"/> No					
Astrovirus		<input type="checkbox"/> Yes <input type="checkbox"/> No					
Enterotoxigenic <i>E. coli</i> (ETEC) <i>lt/st</i>		<input type="checkbox"/> Yes <input type="checkbox"/> No					
<i>Entamoeba histolytica</i>		<input type="checkbox"/> Yes <input type="checkbox"/> No					
<i>Clostridium difficile</i> Toxin A/B		<input type="checkbox"/> Yes <input type="checkbox"/> No					
<i>Vibrio</i> ( <i>V. parahaemolyticus</i> , <i>V. vulnificus</i> , and <i>V. cholerae</i> )		<input type="checkbox"/> Yes <input type="checkbox"/> No					
<i>Campylobacter</i> ( <i>C. jejuni</i> , <i>C. coli</i> , and <i>C. upsaliensis</i> )		<input type="checkbox"/> Yes <input type="checkbox"/> No					
Shiga-like toxin-producing <i>E. coli</i> (STEC) <i>stx1/stx2</i>		<input type="checkbox"/> Yes <input type="checkbox"/> No					
<i>E. coli</i> O157		<input type="checkbox"/> Yes <input type="checkbox"/> No					
Rotavirus A		<input type="checkbox"/> Yes <input type="checkbox"/> No					
<i>Giardia lamblia</i>		<input type="checkbox"/> Yes <input type="checkbox"/> No					
<i>Plesiomonas shigelloides</i>		<input type="checkbox"/> Yes <input type="checkbox"/> No					
<i>Yersinia enterocolitica</i>		<input type="checkbox"/> Yes <input type="checkbox"/> No					

Reviewed by: \_\_\_\_\_  
Signature Date